



Replacement Sheet

Head-Stabilized Medical Apparatus, System and Methodology

Serial No. 10/715,871

John M. Epley
Page 1 of 5



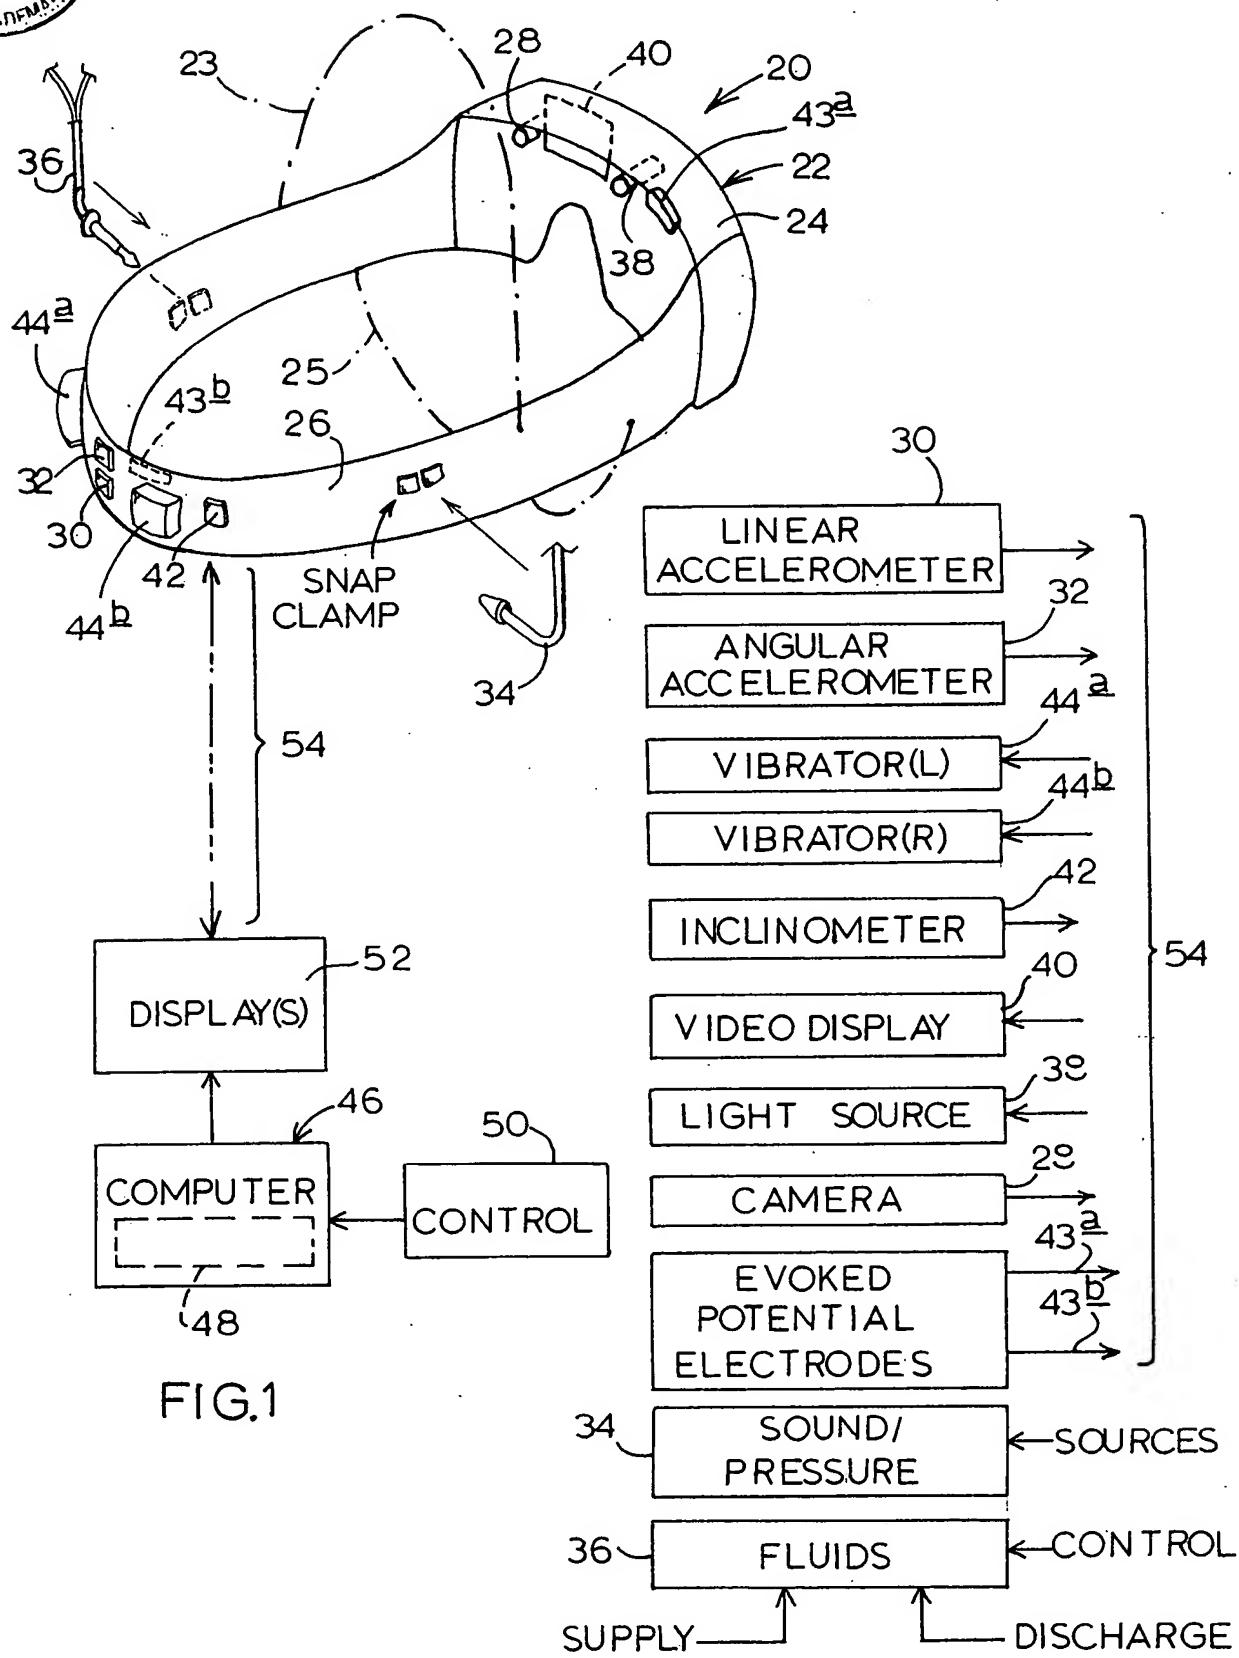


FIG.1

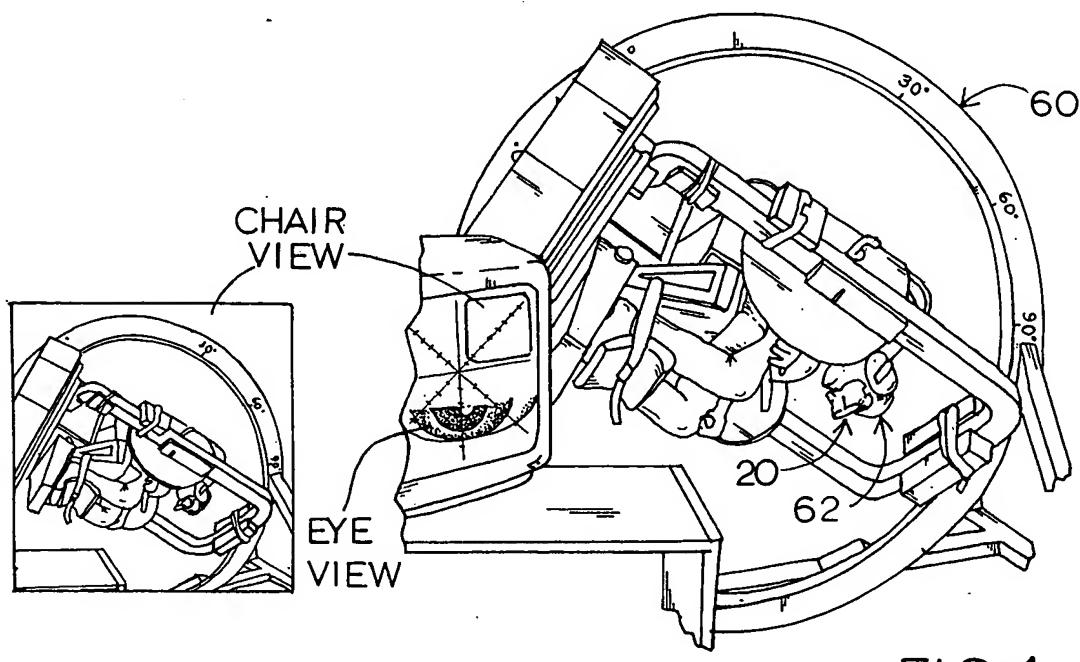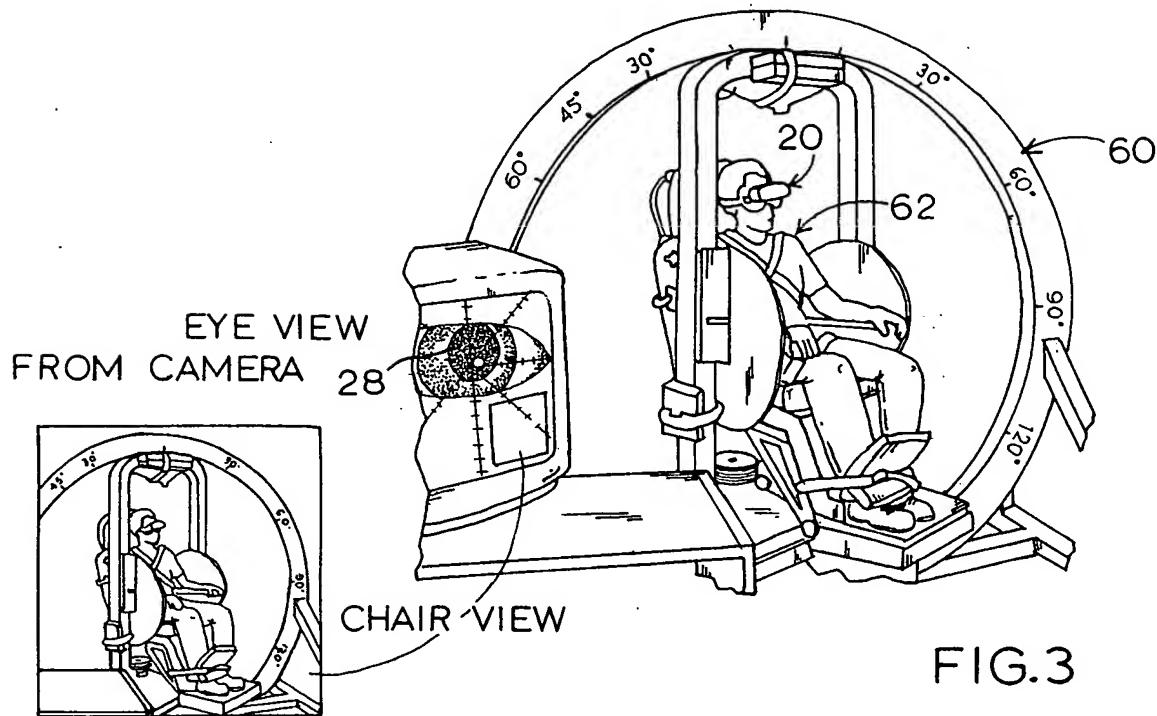

Replacement Sheet

Head-Stabilized Medical Apparatus, System and Methodology

Serial No. 10/715,871

John M. Epley

Result: **CW torsional nystagmus** Latency 3.5 sec Duration:11.2 sec Dx: **Canalithiasis of Left PSC**

Advice: Continue with Epley Maneuver. GO TO: Position 2 V/A: left roll, rate 7°/sec GO? Y/N

५०

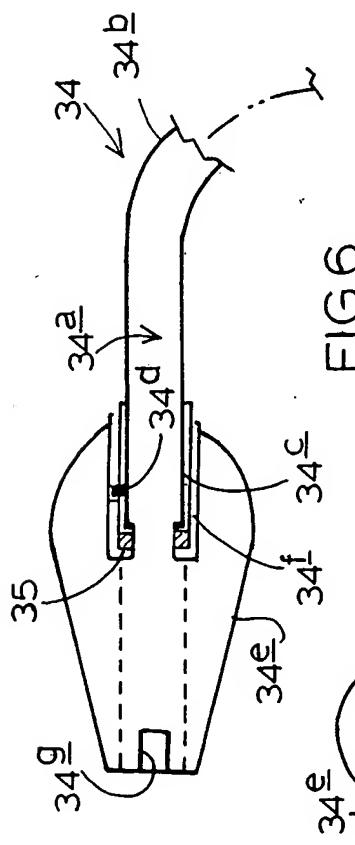


FIG. 6

FIG. 7

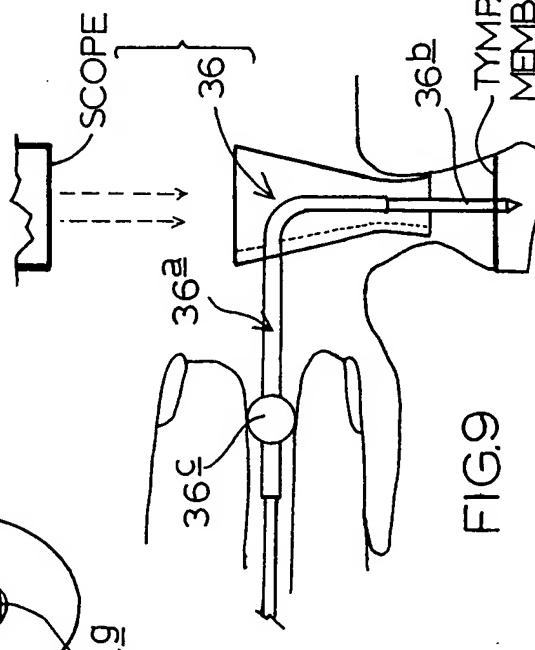


FIG. 9

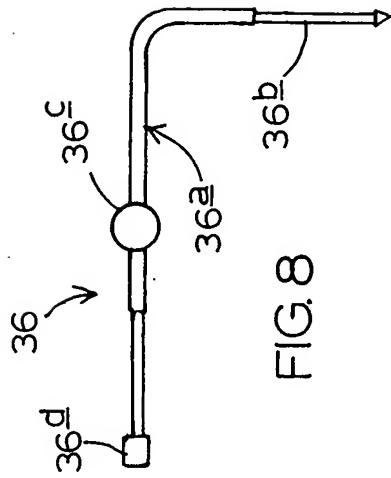


FIG. 8

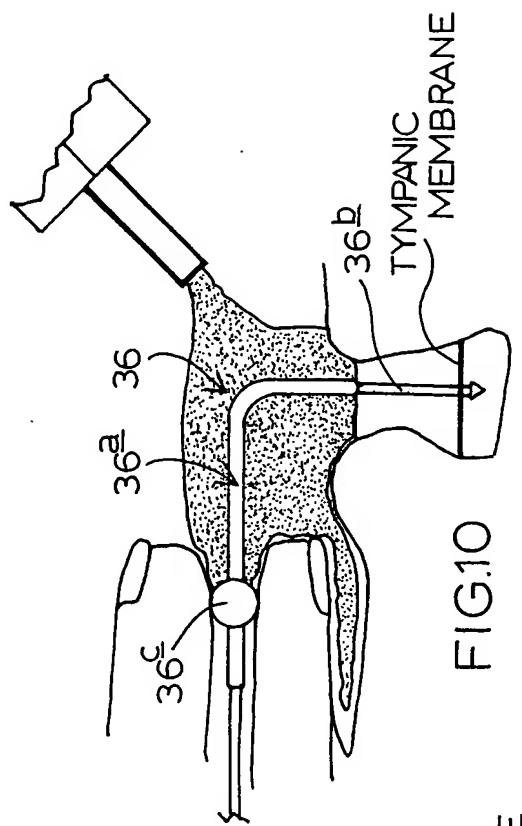


FIG. 10

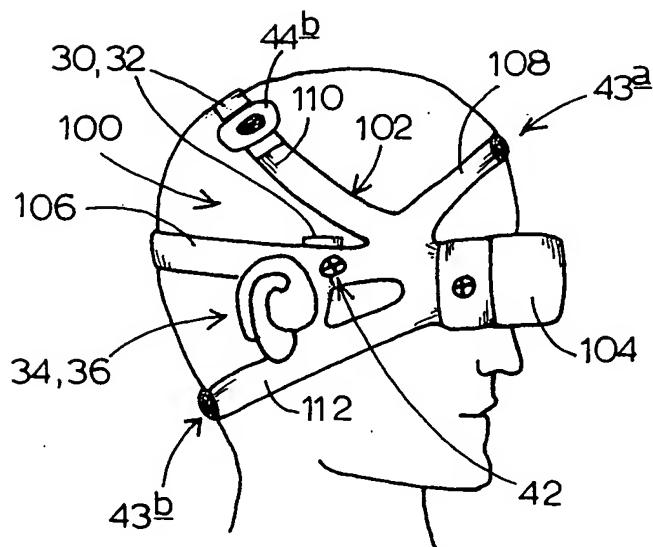


FIG.11

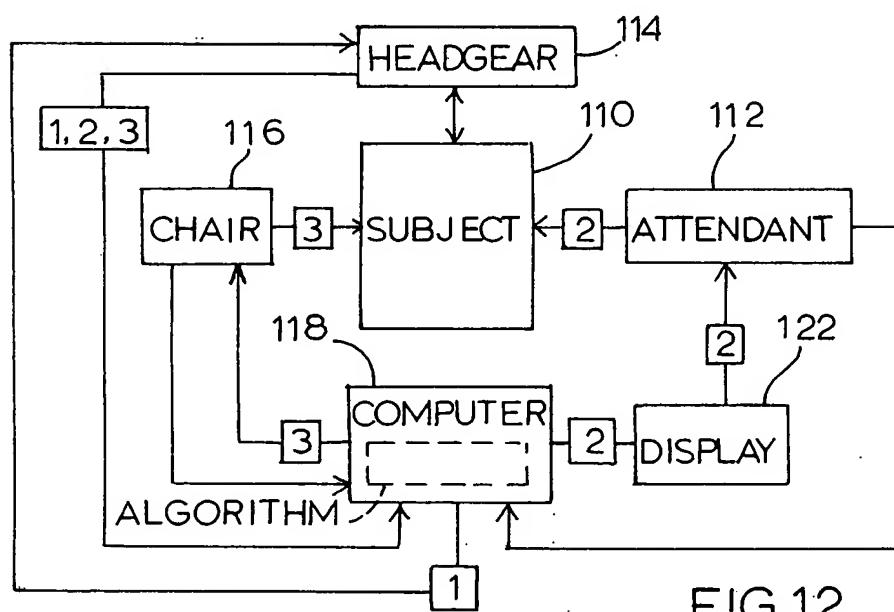


FIG.12